

# Ordering Information

## CAPTIVATOR™ II POLYPECTOMY SNARES

Order Number	Description	Stiffness	Loop Width (mm)	Sheath O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00561221	10mm <b>Rounded</b>	Stiff	10	2.4	240	2.8	Box 10
M00561222	10mm <b>Rounded</b>	Stiff	10	2.4	240	2.8	Box 20
M00561223	10mm <b>Rounded</b>	Stiff	10	2.4	240	2.8	Box 40
M00561231	15mm <b>Rounded</b>	Stiff	15	2.4	240	2.8	Box 10
M00561232	15mm <b>Rounded</b>	Stiff	15	2.4	240	2.8	Box 20
M00561233	15mm <b>Rounded</b>	Stiff	15	2.4	240	2.8	Box 40
M00561241	20mm <b>Rounded</b>	Stiff	20	2.4	240	2.8	Box 10
M00561242	20mm <b>Rounded</b>	Stiff	20	2.4	240	2.8	Box 20
M00561243	20mm <b>Rounded</b>	Stiff	20	2.4	240	2.8	Box 40
M00561191	25mm <b>Rounded</b>	Stiff	25	2.4	240	2.8	Box 10
M00561192	25mm <b>Rounded</b>	Stiff	25	2.4	240	2.8	Box 20
M00561193	25mm <b>Rounded</b>	Stiff	25	2.4	240	2.8	Box 40
M00561291	33mm <b>Rounded</b>	Stiff	33	2.4	240	2.8	Box 10

## CAPTIVATOR™ POLYPECTOMY SNARES

Order Number	Description	Stiffness	Loop Width (mm)	Sheath O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00562301	Small <b>Oval</b>	Stiff	13	2.4	240	2.8	Box 10
M00562321	Medium <b>Oval</b>	Stiff	27	2.4	240	2.8	Box 10
M00562391	Large <b>Oval</b> (thin wire)	Flexible	30	2.4	240	2.8	Box 10
M00561311	Large <b>Oval</b>	Medium Stiff	30	2.4	240	2.8	Box 10
M00562451	Small <b>Hexagonal</b>	Stiff	13	2.4	240	2.8	Box 10
M00562341	Medium <b>Hexagonal</b>	Stiff	27	2.4	240	2.8	Box 10
M00562371	Medium <b>Crescent</b>	Stiff	27	2.4	240	2.8	Box 10

## ROTATABLE SNARES\*

Order Number	Description	Stiffness	Loop Width (mm)	Sheath O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00561821	Small <b>Oval</b>	Medium Stiff	13	2.4	195	2.8	Box 10
M00561831	Medium <b>Oval</b>	Medium Stiff	20	2.4	195	2.8	Box 10

\*With Star Catheter Technology

## SENSATION™ POLYPECTOMY SNARES - SHORT THROW HANDLE SNARES

Order Number	Description	Stiffness	Loop Width (mm)	Sheath O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00562691	Small <b>Oval</b>	Flexible	13	2.4	240	2.8	Box 5
M00562692	Small <b>Oval</b>	Flexible	13	2.4	240	2.8	Box 20
M00562693	Small <b>Oval</b>	Flexible	13	2.4	240	2.8	Box 40
M00560321	Small <b>Oval</b>	Medium Stiff	13	2.4	240	2.8	Box 5
M00562671	Medium <b>Oval</b>	Flexible	27	2.4	240	2.8	Box 5
M00562672	Medium <b>Oval</b>	Flexible	27	2.4	240	2.8	Box 20
M00562673	Medium <b>Oval</b>	Flexible	27	2.4	240	2.8	Box 40
M00560311	Medium <b>Oval</b>	Medium Stiff	27	2.4	240	2.8	Box 5
M00562651	Large <b>Oval</b>	Medium Stiff	30	2.4	240	2.8	Box 5
M00562652	Large <b>Oval</b>	Medium Stiff	30	2.4	240	2.8	Box 20
M00560331	Medium <b>Crescent</b>	Medium Stiff	27	2.4	240	2.8	Box 5

## CAPTIFLEX™ POLYPECTOMY SNARES

Order Number	Description	Stiffness	Loop Width (mm)	Sheath O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00562471	Extra Small <b>Oval</b>	Flexible	11	2.4	240	2.8	Box 10
M00562421	Small <b>Oval</b>	Flexible	13	2.4	240	2.8	Box 10
M00562422	Small <b>Oval</b>	Flexible	13	2.4	240	2.8	Box 40
M00562401	Medium <b>Oval</b>	Flexible	27	2.4	240	2.8	Box 10
M00562402	Medium <b>Oval</b>	Flexible	27	2.4	240	2.8	Box 40

## PROFILE™ POLYPECTOMY SNARES - PEDIATRIC SNARES


Order Number	Description	Stiffness	Loop Width (mm)	Sheath O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00562531	Extra Small <b>Oval</b>	Flexible	11	1.9	240	2.0	Box 10
M00562551	Small <b>Oval</b>	Flexible	13	1.9	240	2.0	Box 10
M00562571	Medium <b>Oval</b>	Flexible	27	1.9	240	2.0	Box 10

## TWISTER® PLUS ROTATABLE RETRIEVAL DEVICE

Order Number	Description	Loop Width (mm)	Sheath O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00561411	TWISTER PLUS Rotatable Retrieval Device	22	2.5	230	2.8	Box 5
M00561412	TWISTER PLUS Rotatable Retrieval Device	22	2.5	230	2.8	Box 10
M00561421	TWISTER PLUS Rotatable Retrieval Device	26	2.5	230	2.8	Box 5
M00561422	TWISTER PLUS Rotatable Retrieval Device	26	2.5	230	2.8	Box 10

## RADIAL JAW™ 4 HOT BIOPSY FORCEPS

Order Number	Description	Jaw O.D. (mm)	Working Length (cm)	Min. Working Channel (mm)	Units
M00515031	Radial Jaw 4 Hot Biopsy Forceps	2.2	240	2.8	Box 5
M00515032	Radial Jaw 4 Hot Biopsy Forceps	2.2	240	2.8	Box 20
M00515033	Radial Jaw 4 Hot Biopsy Forceps	2.2	240	2.8	Box 40

 These products are for single use only. Do not reuse.

All cited trademarks are the property of their respective owners. CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labeling supplied with each device. Information for the use only in countries with applicable health authority product registrations.

TWISTER® PLUS is a trademark of Horizons International Corp. Distributed by Boston Scientific Corporation, Natick, Massachusetts; manufactured by Horizons International Corp., Heredia, Costa Rica.

ENDO-262202-AA Aug 2014. Printed in The Netherlands by DeBudelse/creativeservices.

**Boston Scientific**

Advancing science for life™

www.bostonscientific-international.com

© 2014 Boston Scientific Corporation or its affiliates. All rights reserved. DINEND2330EA

# Tissue Resection Devices

**Boston Scientific**



## TWISTER® PLUS Rotatable Retrieval Device

Three dimensional net device that is fully rotatable and designed to facilitate retrieval of polyps, EMR/ESD fragments, food bolus and foreign bodies.

### Nylon Retrieval Net

- Designed to ensure retention of bodies

### 360° Rotation (1:1 ratio to both directions)

- Designed to facilitate and shorten the procedure with minimal scope manipulation

### Three Dimensional Net


- Designed to allow to scoop the bodies to be retrieved

### Short Throw Handle

- Designed for nurse and technician comfort

### Interwoven Net Design

- Net is attached to the outer wire using an interwoven design to help maintain the integrity of the net

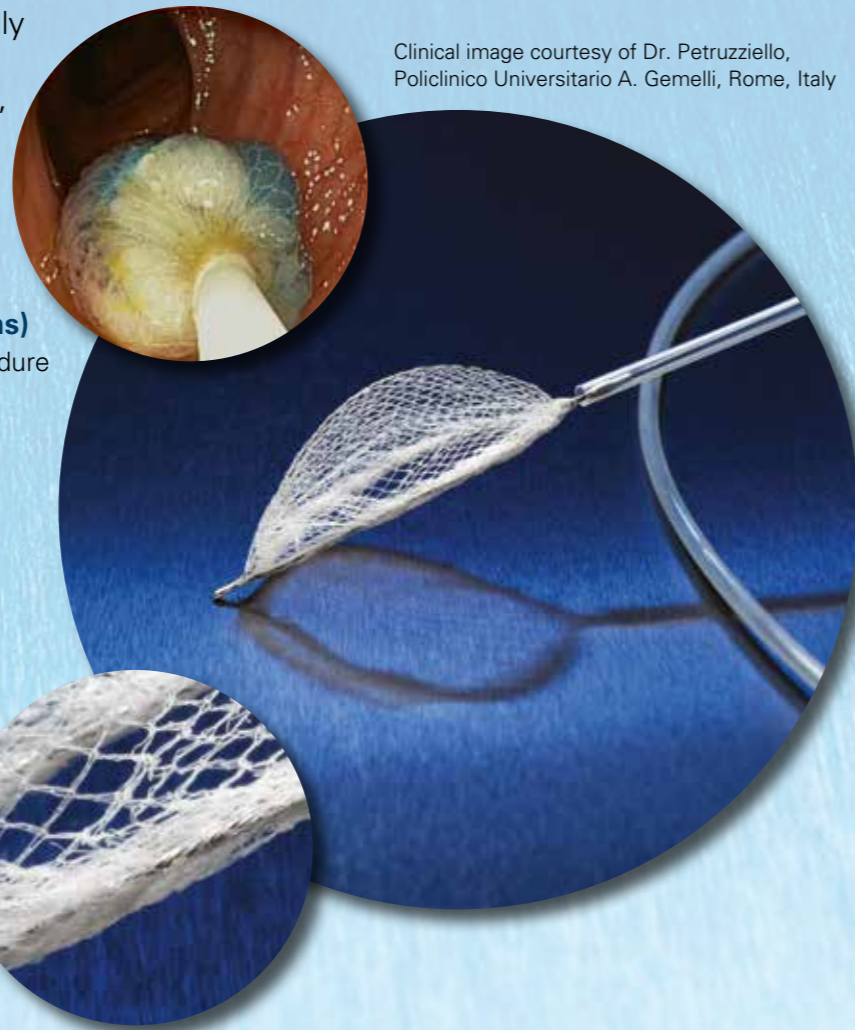

Clinical image courtesy of Dr. Petruzzello, Policlinico Universitario A. Gemelli, Rome, Italy

## Radial Jaw™ 4 Hot Biopsy Forceps

Hot forceps available in our family of market-leading single-use biopsy forceps.

### Jaw Configuration

*Designed to provide:*

- Tissue specimens for excellent sample handling, preparation and accurate histological diagnosis
- Enhanced passability through tortuous anatomy

### Micro-Mesh Tooth Design

- Engineered for a clean, precise bite

### Streamlined Catheter

- Designed to provide the right balance of columnar strength and flexibility for excellent pushability and control during scope passage

### Positioning Markers

- Engineered to assist in the insertion and withdrawal of forceps to enhance procedural safety and efficiency



## Polypectomy Snares

Available in a broad range of loop sizes and shape configurations. All of them approved for both hot and cold snaring.

### Captivator™ II Snare

- Rounded shape to facilitate polyps and mucosal resection. Short distance from scope tip designed for visualization and tip control

### Captivator™ Snare

- Offers a variety of snare loop configurations to accommodate a wide range of therapeutic functions

### Rotatable Snare

- Designed to provide 360° rotation to help access difficult polyps

### Sensation™ Short Throw Handle Snare

- Short throw handle is designed for nurse and technician comfort

### Captiflex™ Snare

- Incorporates a braided wire design engineered to produce a flexible snare

### Profile™ Pediatric Snare

- Engineered to fit through most 2.0mm pediatric working channels



New ergonomic handle for the new Captivator™ II sizes: 10, 15, 20, 25mm

